



Installation Instructions

Panel Cutout: 182 x 94 mm

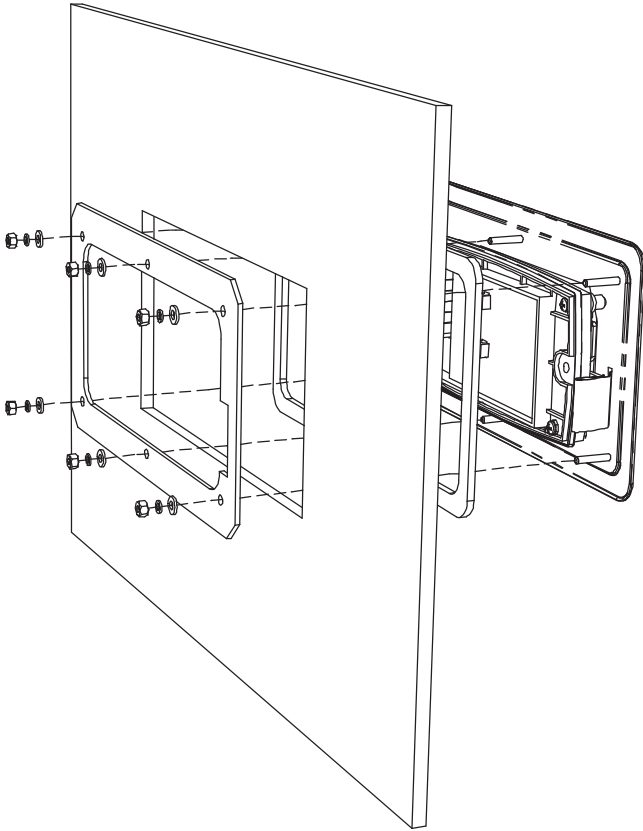

Caution:

- Ensure keypad tail is kept clear of cutout.
- Ensure panel gasket is aligned properly before tightening the panel clamp.
- Gasket may not be re-useable. Replace gasket if thickness is less than 2mm.

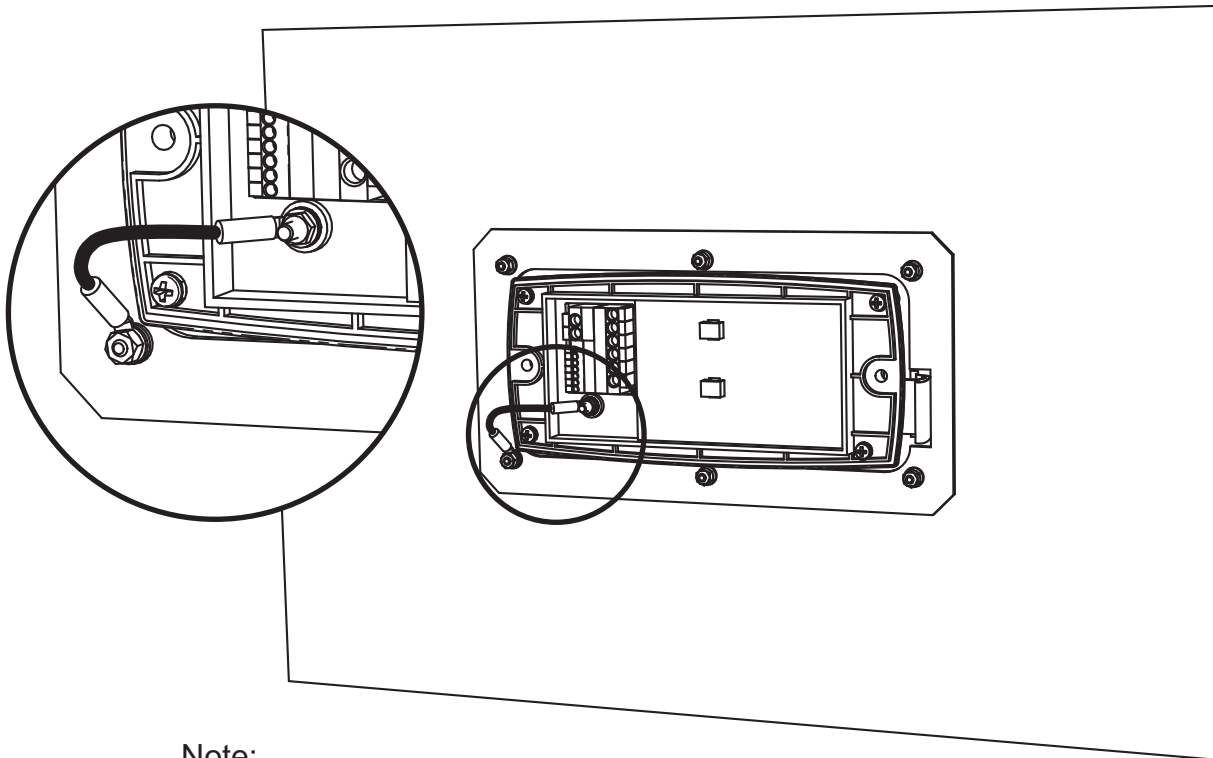

Note:

- It is important that the earth lead supplied is firmly connected to the metal housing as shown. Failure to do so may reduce the instrument's immunity to static discharge.